

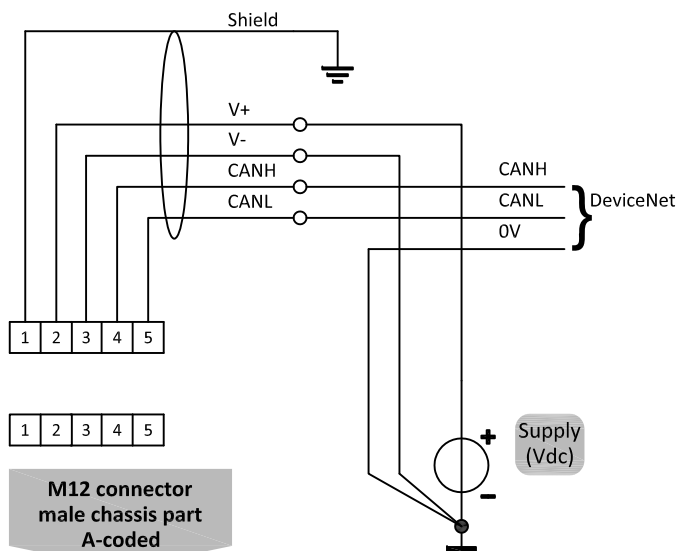
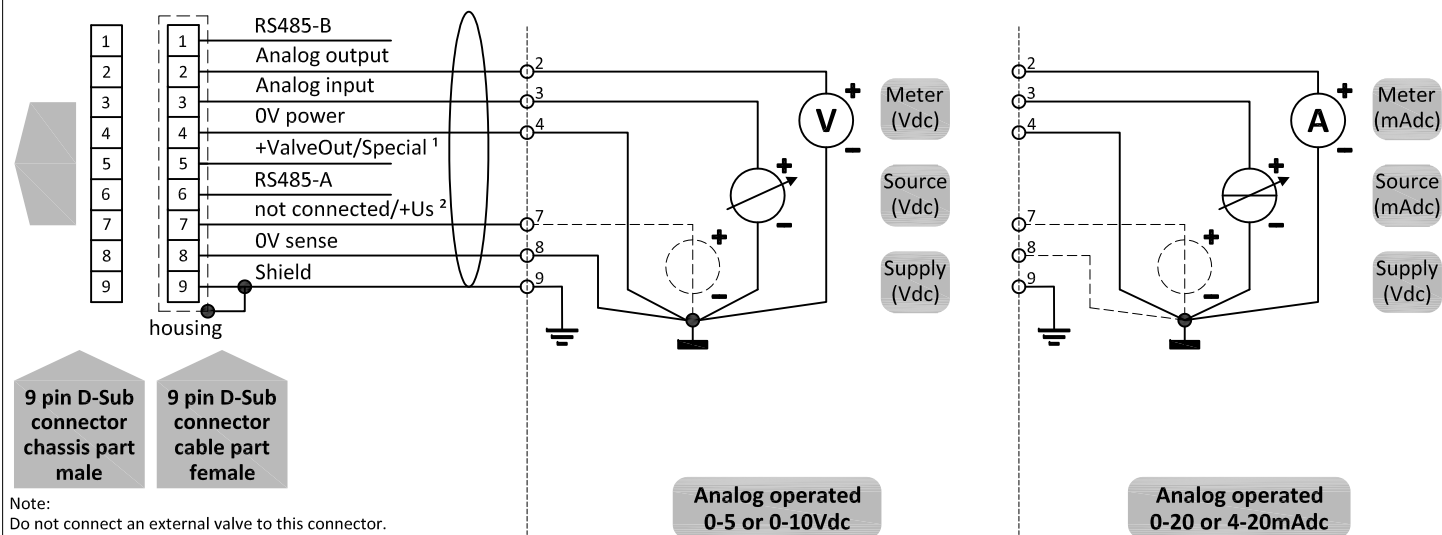


## DeviceNet connection

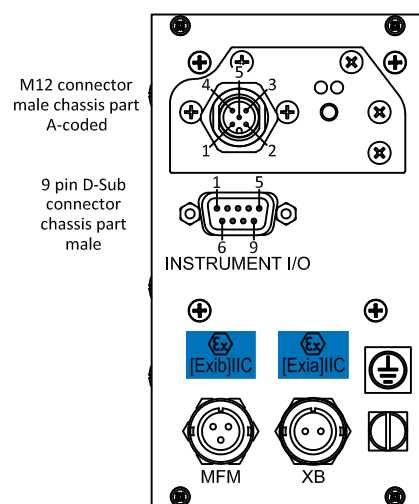

### Model key explanation

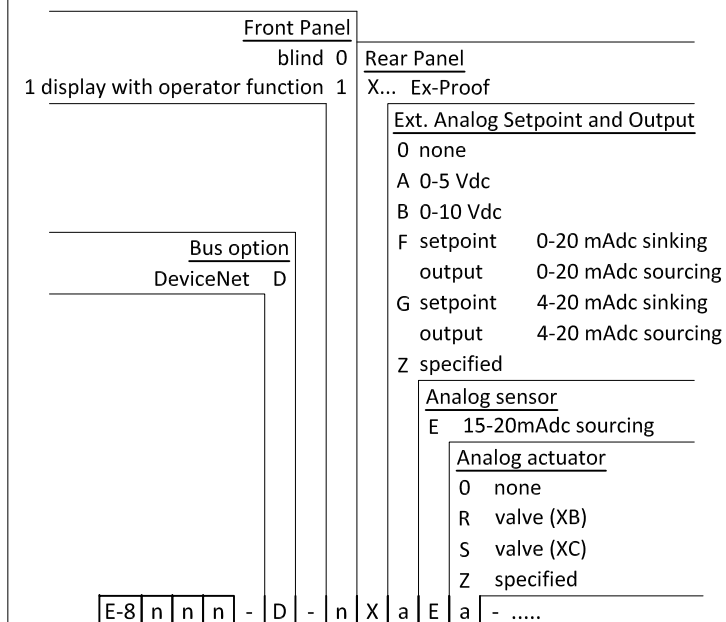

Note: Shown image is Control unit E-8000-D-nXaER.

Note:  
Do not connect an external valve to this connector.

Note:  
1) +Valve out is 0...10Vdc 1mA.  
2) For stand alone version: External power supply (+Us) = 24Vdc  $\pm 10\%$ .

Note:  
When using a field bus or RS232, it is not possible to operate the instrument by using the setpoint signal of the analog D-sub connector without changing the value of parameter "control mode". See doc.nr. 9.17.023 for more details.