

Bronkhorst®

doc.nr.: 9.16.365A
date: 26-10-2026

RS485 interfaces
Modbus (ASCII & RTU) / FLOW-BUS / ProPar

Hook-up diagram
CORI-FLOW
M15 MKII

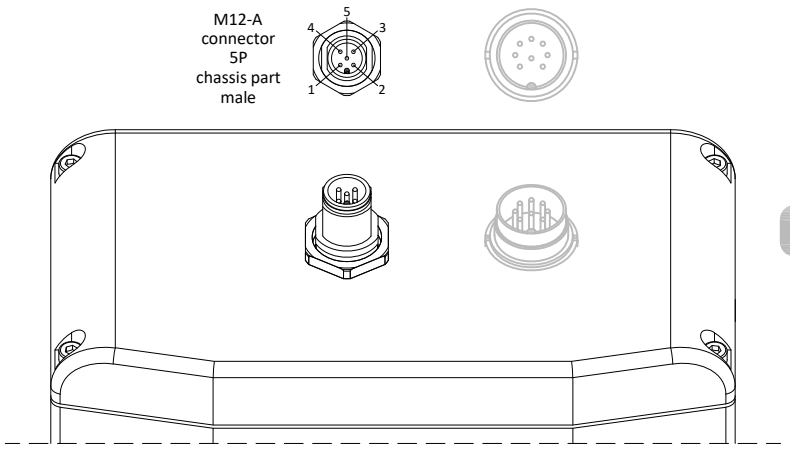

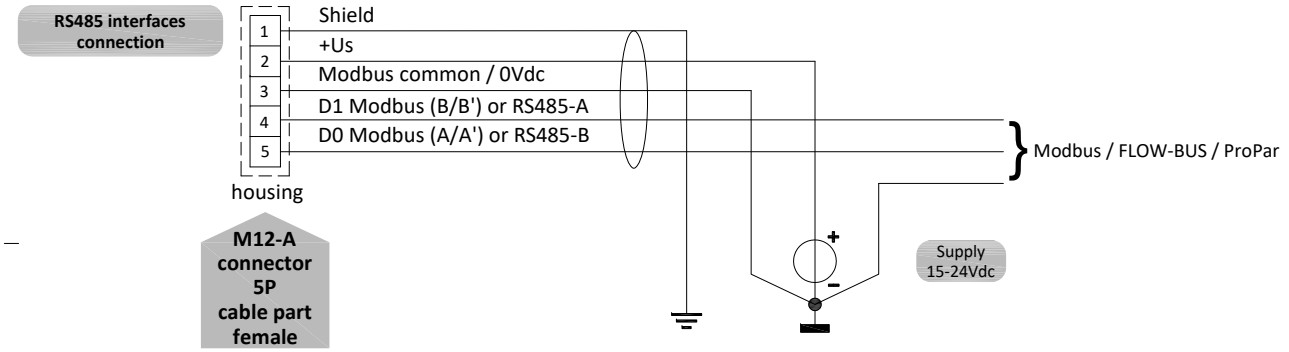

For reliable measurements, it is important to reduce interference from outside noise on the signals.

- When connecting to other devices, ensure that the integrity of the shielding is maintained.
- Use shielded cables and wire terminals.