


**DeviceNet connection**

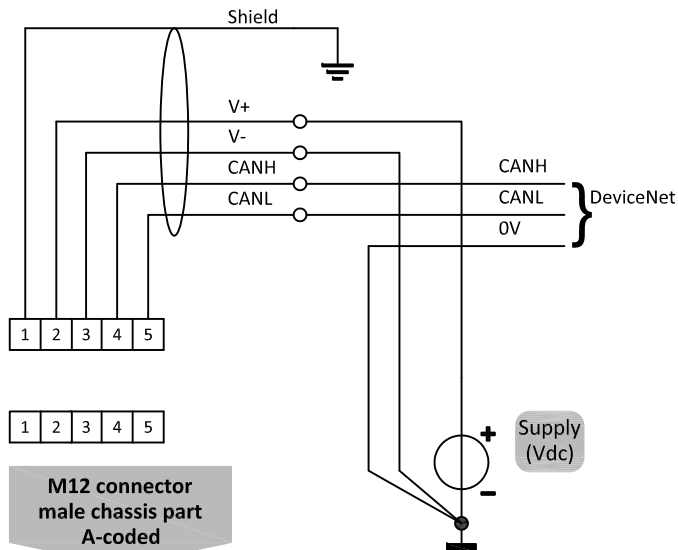

**Model key explanation**

Front Panel

- 0 Blind
- 1 1 Display with operator function

Rear Panel

W... CEM

Ext. Analog Setpoint and Output

- 0 none
- A 0-5 Vdc
- B 0-10 Vdc
- F 0-20 mAdc sourcing
- G 4-20 mAdc sourcing
- Z specified

Analog sensor

- T PT100 Temperature
- Z specified



Analog actuator

- U W100/W200
- V W300
- Z specified



M12 connector male chassis part A-coded

9 pin D-Sub connector chassis part male

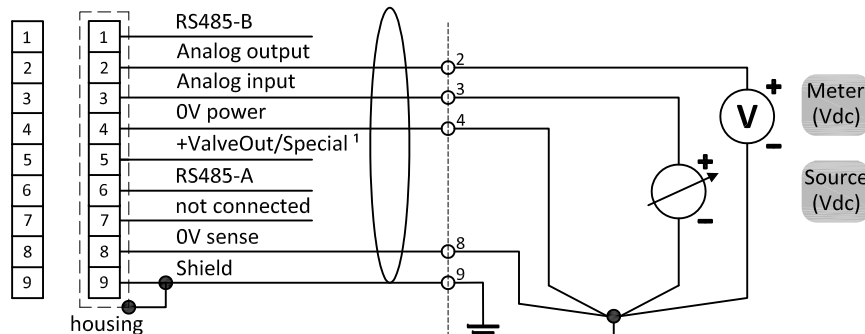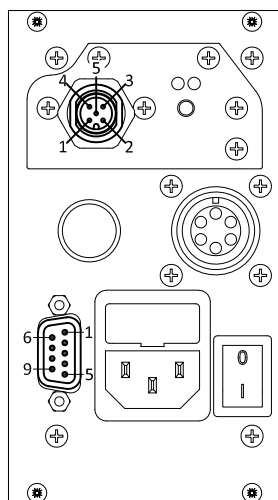

9 pin D-Sub connector chassis part male


9 pin D-Sub connector cable part female

Note:  
Do not connect an external valve to the instrument.

Note:  
<sup>1</sup>) +Valve out is 0-10Vdc 1mA.

**Analog operated  
0-5 or 0-10Vdc**

Note:  
When using a field bus or RS232, it is not possible to operate the instrument by using the setpoint signal of the analog D-sub connector without changing the value of parameter "control mode". See doc.nr. 9.17.023 for more details.

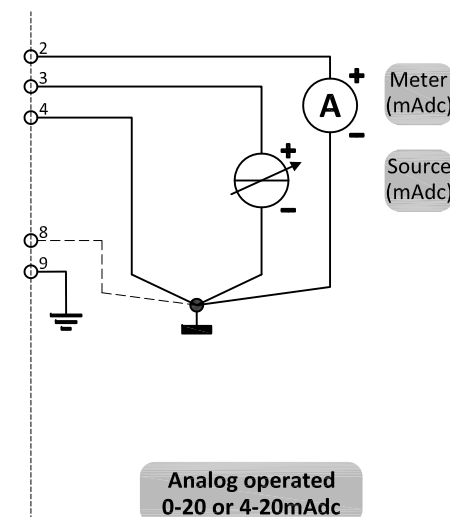

**Analog operated  
0-20 or 4-20mAdc**